


NOTE-CIRCUIT IS NOT GROUNDED TO CHASSIS, GROUND OBTAINED FROM EXPANDER UNIT.  
 NOTE-BOXED WORDS ARE LABELS.  
 NOTE-ALLOW THE POWER SUPPLY 5 MINUTES TO DISCHARGE AFTER RUNNING WITHOUT LOAD. SHORTING OUTPUT MAY BLOW METER FUSE.

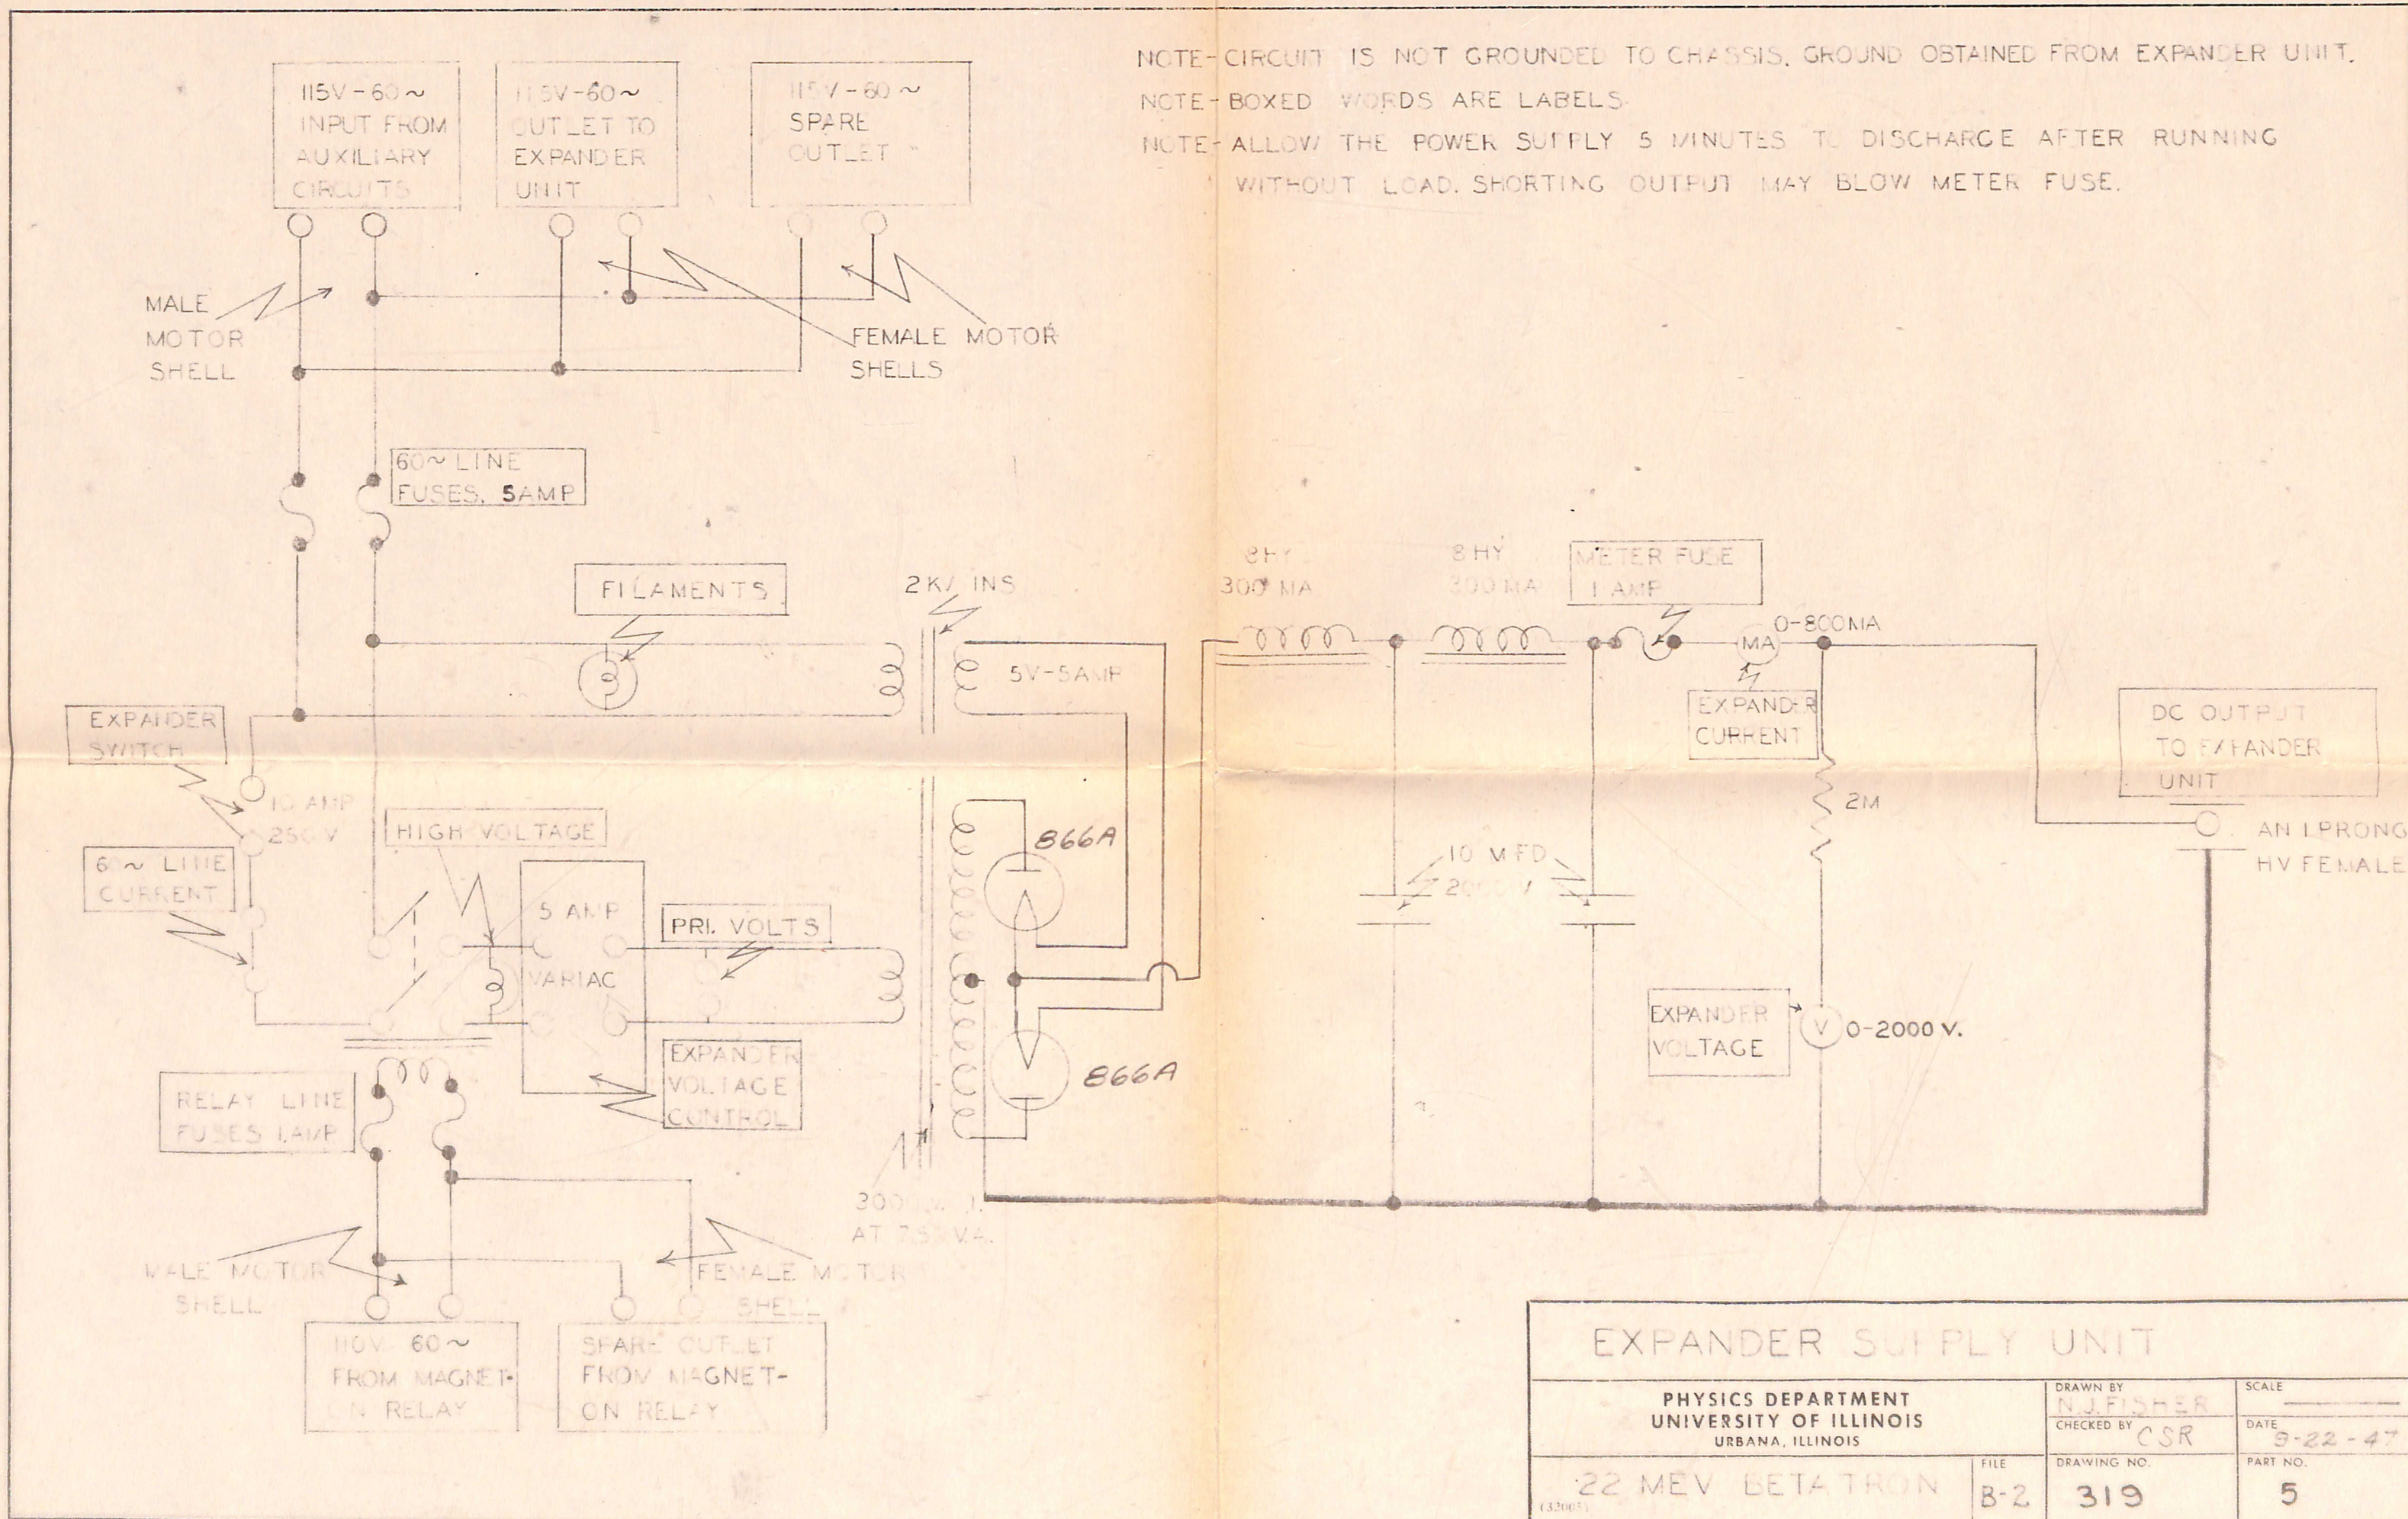

EXPANDER SUPPLY UNIT			
PHYSICS DEPARTMENT UNIVERSITY OF ILLINOIS URBANA, ILLINOIS	DRAWN BY N.J. FISHER	SCALE	
	CHECKED BY CSR	DATE	9-22-47
22 MEV BETA TRON <small>(32003)</small>	FILE B-2	DRAWING NO. 319	PART NO. 5

5 prints